





Microphone Frequency Response Measurement Report

Microphone Manufacturer: miniDSP **Model Number:** UMIK-1
Serial Number: 700-0589 **Phantom Power:** USB

Measurement Date: May 12, 2013 **Temperature:** 72°F/22°C
Engineer: H. Singleton **Humidity:** 46%

1/3 OB Results	
Freq.	Resp. (dB)
5	-5.31
6.3	-3.99
8	-2.74
10	-1.52
12.5	-0.51
16	0.23
20	0.74
25	1.06
31.5	1.25
40	1.36
50	1.40
63	1.39
80	1.36
100	1.31
125	1.29
160	1.27
200	1.24
250	1.09
315	0.78
400	0.57
500	0.34
630	0.22
800	0.16
1000	0.00
1250	-0.14
1600	-0.09
2000	0.13
2500	0.30
3150	0.66
4000	1.18
5000	1.77
6300	2.10
8000	2.32
10000	2.26
12500	1.32
16000	0.16
20000	-6.01
25000	-68.06

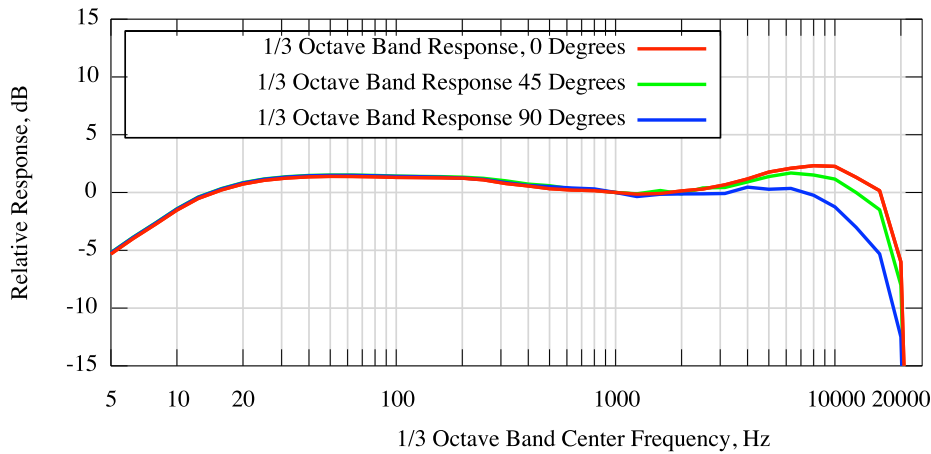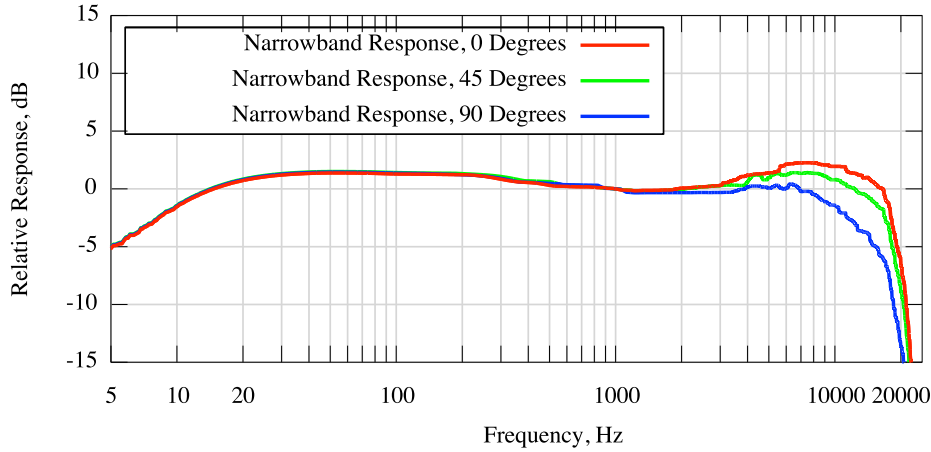

This frequency response measurement is not a NIST-traceable calibration.

Reference Microphone

Ref. Microphone Frequency Response: ACO Pacific 7052E, S/N 54478

